

Determination of Cross Sections by Overtone Mobility Spectrometry: Evidence for Loss of Unstable Structures at Higher Overtones

Sunyoung Lee, Michael A. Ewing, Fabiane M. Nachtigall,[†] Ruwan T. Kurulugama,[‡] Stephen J. Valentine,^{*} and David E. Clemmer^{*}

Department of Chemistry, Indiana University, Bloomington, Indiana 47405

Received: June 29, 2010; Revised Manuscript Received: August 16, 2010

Overtone mobility spectrometry (OMS) is examined as a means of determining the collision cross sections for multiply charged ubiquitin and substance P ions, as well as for singly charged raffinose and melezitose ions. Overall, values of collision cross section measured by OMS for stable ion conformations are found to be in agreement with values determined by conventional ion mobility spectrometry (IMS) measurements to within $\sim 1\%$ relative uncertainty. The OMS spectra for ubiquitin ions appear to favor different conformations at higher overtones. We propose that the changes in the distributions as a function of the overtone region in which they are measured arise from the elimination of ions that undergo structural transitions in the drift regions. Kinetics simulations suggest that structural transitions occurring on the order of a few ms and resulting in an $\sim 4\%$ change in ion collision cross sections are detected by OMS measurements. The unique method of distinguishing ion mobilities with OMS reveals these structural transitions which are not readily apparent from traditional IMS measurements.

Introduction

Overtone mobility spectrometry (OMS)^{1,2} is a gas-phase separation method that filters ions according to differences in mobilities through an inert buffer gas. Selection is achieved by applying time-dependent fields to drift tube segments creating periodic ion elimination regions. Ions with mobilities that are resonant with the field application frequency pass through these regions and are transmitted to the detector. Measurement of ion intensity as field application frequency is scanned generates the OMS spectrum. While the method is very similar to IMS, there are some interesting differences. First, because transmission is based on the drift field application frequency, no initial pulse is required to initiate experiments. Instead, the beam emerges as pulses of ions that remained stable throughout the drift region. Additionally, because the approach is based on the elimination of ions, the OMS resolving power (R_{OMS}) scales with the number of drift regions. Thus, whereas the resolving power for IMS (R_{IMS}) is proportional to the square root of the drift tube length, theory and experiments show that OMS resolving power scales in a roughly linear fashion with length.^{1,2}

Because OMS measurements are carried out using weak, uniform fields and the basis of ion selection is mobility matching with the field application frequency, ions of specific cross sections can be transmitted by fixing the frequency of the applied drift field. The relationship of the ion cross section to the drift field frequency is given by²

$$\Omega = \frac{(18\pi)^{1/2}}{16} \frac{ze}{(k_{\text{b}}T)^{1/2}} \left[\frac{1}{m_{\text{I}}} + \frac{1}{m_{\text{B}}} \right]^{1/2} \frac{E[\phi(h-1) + 1] 760}{f(l_{\text{I}} + l_{\text{e}})} \frac{T}{P} \frac{1}{273.2N} \quad (1)$$

In eq 1, k_{b} , z , e , N , T , and P correspond to Boltzmann's constant, the ion's charge, the charge of an electron, the neutral number density, and the temperature and pressure of the buffer gas, respectively. The parameters E , m_{I} , and m_{B} represent the electric field and the masses of the ion and buffer gas, respectively. Other variables include the OMS parameters field application frequency (f), operational phase (ϕ), harmonic index (h), and ion transmission (l_{I}) and elimination (l_{e}) region lengths. For comparisons of features in OMS (and IMS) data sets (especially when values of z and m are not known), it is useful to report reduced mobilities (K_0) using the relationship shown in eq 2.

$$K_0 = \frac{f(l_{\text{I}} + l_{\text{e}})}{E[\phi(h-1) + 1] 760} \frac{P}{T} \frac{273.2}{T} \quad (2)$$

From an understanding of how OMS and IMS measurements are carried out, one predicts that the distributions that are measured may show different features. For example, if an ion undergoes structural transitions as it migrates through a drift tube, the IMS approach would record the average drift time associated with all structures that were sampled during the time in the drift tube. On the other hand, if ions change structure during an OMS experiment, the new structure may not be mobility matched with the field frequency. Thus, we expect new structures, having nonresonant mobilities, to be eliminated. Here, we investigate the ability of OMS measurements to provide reliable structural information as ion collision cross sections. Overall, good agreement between OMS and IMS measurements is observed. However, examination of OMS spectra reveals that some features in OMS distributions are not observed in higher

^{*} Author to whom correspondence should be addressed. E-mail: clemmer@indiana.edu.

[†] Current address: State University of Campinas, CP 6154 CEP 13084-862, Campinas, SP, Brazil.

[‡] Current address: Pacific Northwest National Laboratory, Richland, WA 99352.

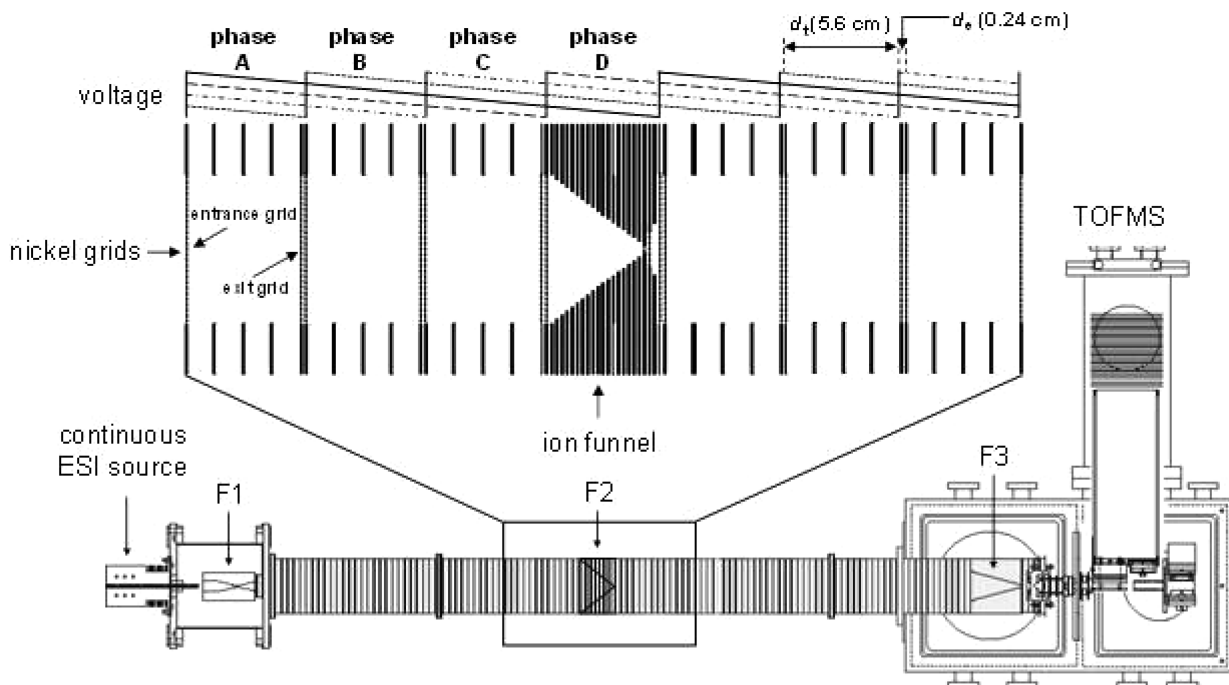


Figure 1. Schematic diagram of the OMS-TOF instrument used to measure the collision cross section distributions. The drift tube assembly consists of three ion funnels (F1–F3) and multiple segmented drift regions (22 sections). The segmented regions are divided by lenses containing nickel mesh grids. Each section is operated using an electric field of $9 \text{ V} \cdot \text{cm}^{-1}$ (ion transmission region, 5.6 cm). Periodic repulsive fields of $963 \text{ V} \cdot \text{cm}^{-1}$ are created between specific sets of grids (d_e regions, 0.24 cm). The four-phase system applied in these studies utilizes four distinct drift field settings (phases A, B, C, and D). These fields are modulated at different frequencies to allow the ions with appropriate mobilities to move through the drift tube.

frequency spectral regions. It appears that the loss of these ions arises because structural transitions lead to a mismatch in mobility and field application frequency. Simulations suggest that such structural transitions occur on the ms time scale, supporting results obtained from earlier studies of protein ions.^{3–5}

Since the introduction of electrospray ionization (ESI),⁶ a number of experiments designed to study macromolecular ion structures have been presented.^{7–28} There is substantial interest in understanding transitions between conformational states. The development of a technique that allows transmission of stable structures would be useful as a means of purifying ions prior to other spectroscopic studies. Other analytical techniques that provide a means of ion filtering based on their mobilities include field asymmetric ion mobility spectrometry (FAIMS)^{29–32} and differential mobility analysis.^{33–37} An advantage of the OMS approach is that accurate collision cross sections can be obtained directly from the measurement. Additionally, an understanding of transitions between states and development of methods that allow unstable states to be eliminated will be valuable in the development of higher resolution mobility measurements.

Experimental Methods

Overview. Detailed descriptions of IMS theory,^{38–42} instrumentation,^{43–48} and techniques^{26,49–51} are described elsewhere. Additionally, details regarding the OMS method and instrument as well as the general theory behind OMS measurements have been reported.^{1,2} Here, only a brief description of the OMS instrument and its operational mode used for these studies is given. Figure 1 shows a schematic diagram of the experimental apparatus. The OMS instrument includes an ESI source, a drift tube, ion focusing elements, and a time-of-flight (TOF) mass spectrometer. Direct infusion of the analyte solution through a pulled-tip capillary maintained at 2200 V relative to the ESI source entrance generates the protonated ions. Ions are focused

into a drift tube through an ion funnel (F1) interface.^{52,53} Ions are then transmitted through a portion of the drift tube under the influence of a uniform electric field ($9 \text{ V} \cdot \text{cm}^{-1}$) maintained at a pressure of ~ 2.95 Torr of 300 K He buffer gas. Ions exiting the OMS region drift through the rest of the drift tube and are extracted into the TOF instrument for mass analysis.

OMS-MS Instrumentation: General Aspects of OMS. The OMS drift region is comprised of 22 segments (see inset in Figure 1) divided by nickel grids (90% transmittance, Buckbee-Mears, St. Paul, MN). Each segmented region contains both an ion transmission (d_i) and an ion elimination region (d_e). A sawtooth potential gradient is applied to multiple adjoining segmented regions and is modulated between a number of different settings. This generates a uniform DC field ($9 \text{ V} \cdot \text{cm}^{-1}$) across the coupled d_i (5.6 cm long) regions as well as a repulsive field ($963 \text{ V} \cdot \text{cm}^{-1}$) in multiple interfacing d_e (0.24 cm long) regions (see Figure 1). Field modulation causes the repulsive field to shift between alternate d_e regions. Ions with mobilities that do not match the field application frequency eventually locate in one of these d_e regions during transmission, and are neutralized on the wire mesh. Ions with mobilities that are in resonance with the field application frequency are transmitted through the drift tube. Scanning this field application frequency over a relevant range generates a complete OMS distribution.

OMS-MS Instrumentation: Drift Fields Setting in the Segmented Drift Tube. The designated phase (ϕ , the number of distinct field settings) of the OMS instrument defines the mode of operation.^{1,2} For these experiments, fields are created across four contiguous drift tube segments (Figure 1) and are modulated between four different field settings. This mode of operation is identified as a four-phase ($\phi = 4$) system. The field application frequency coinciding with ions of resonant mobilities is termed their fundamental frequency (f_i).^{1,2} The d region ($d_i + d_e$) residence times (and thus the mobilities) of the ions

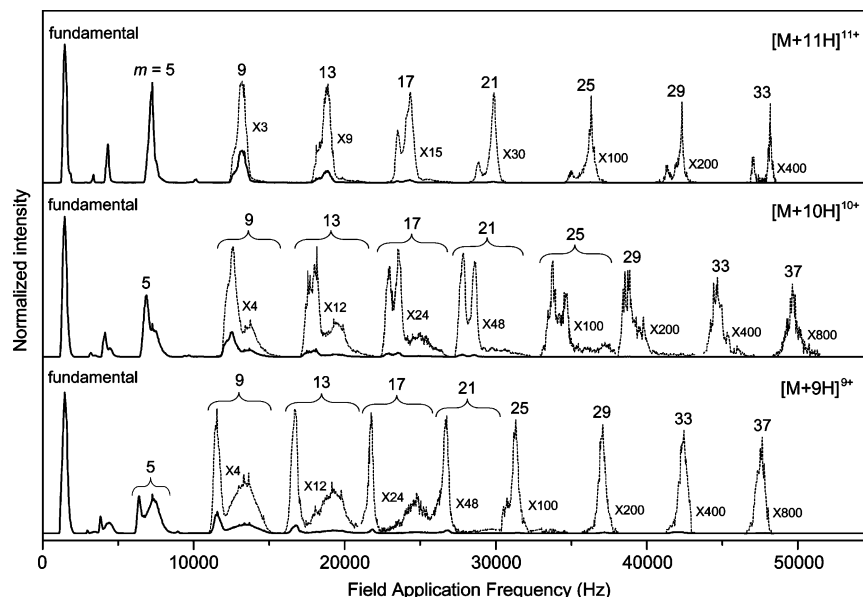


Figure 2. Experimental OMS distributions for the $[M+9H]^{9+}$ to $[M+11H]^{11+}$ charge states of electro sprayed ubiquitin ions. The data are plotted as a function of field application frequency over a range of 0 to 55000 Hz. Low intensity features of each charge state are magnified (dashed lines). m indicates the harmonic frequency number permitting ion transmission (see text for details).

can be determined from OMS spectra. For example, a data set feature with a f_i value of 2000 Hz would require 500 μ s to traverse a single d region. At this frequency, the phase A field (see Figure 1) is activated for a period of 500 μ s; phases B, C, and D are turned off for the same time. After 500 μ s, phase A is turned off and phase B is activated; phases C and D remain unchanged. The field setting shifts from one phase to another every 500 μ s (e.g., $A \rightarrow B \rightarrow C \rightarrow D \rightarrow A \rightarrow \dots$, see Figure 1).

A feature of the OMS system is the observation that transmission of ions is possible at overtone frequencies (f_m) that are exact multiples of the f_i (i.e., $f_m = m \cdot f_i$, where m is the harmonic frequency number).^{1,2} Values of m are defined as $\phi(h-1) + 1$, where h is a positive number termed the OMS harmonic index. For a four-phase system, OMS distribution peaks for a given ion conformation appear at $5 \cdot f_i$, $9 \cdot f_i$, $13 \cdot f_i$, ... frequencies.

OMS Resolving Power. The resolving power of OMS (R_{OMS}) is given by²

$$R_{\text{OMS}} = \frac{1}{1 - \left[1 - \frac{C_2}{R_{\text{IMS}}} \right] \left[\frac{mn - \left[\phi - 1 - \frac{l_c}{l_t + l_e} \right]}{mn} \right]} \quad (3)$$

where n and C_2 correspond with the number of segmented d regions and a correction factor allowing for the relating of R_{OMS} to R_{IMS} , respectively.² While the equation is a little complicated, it does indicate R_{OMS} scales in a nearly linear fashion with the number of drift segments as well as the overtone number.

Experimental Collision Cross Sections. Cross sections from IMS measurements are obtained using³⁹

$$\Omega = \frac{(18\pi)^{1/2}}{16} \frac{ze}{(k_b T)^{1/2}} \left[\frac{1}{m_1} + \frac{1}{m_B} \right]^{1/2} \frac{E 760}{L P} \frac{T}{273.2 N} \quad (4)$$

where t_D and L correspond to the ion's drift time and the drift tube length, respectively. The ability to determine accurate

collision cross sections is governed by how well each parameter is measured experimentally. Because experimental parameters such as buffer gas pressure and temperature and drift field can be precisely controlled, collision cross section measurements of well-characterized systems usually show agreement to within 2% relative uncertainty.⁵⁰ For OMS measurements, field application frequencies are highly tunable and thus comparable levels of precision are achieved.

Sample Preparation. Bovine ubiquitin (90% purity, 76 amino acid residues, $M_r = 8.6$ kDa) was purchased from Sigma (St. Louis, MO) and used without further purification. Multiply charged ubiquitin ions were generated by electro spraying a 2.3×10^{-5} M protein solution dissolved in 49:49:2 (% vol) water: methanol:acetic acid. The sample solution was infused through a pulled capillary (75 μ m i.d., 360 μ m o.d.) tip at a flow rate of 0.3 μ L \cdot min⁻¹ using a syringe pump (KD Scientific, Holliston, MA). A peptide solution (49:49:2% vol, water:methanol:acetic acid) of 1.5×10^{-4} M substance P (98% purity, Sigma) was electro sprayed using identical conditions. Finally, melezitose (99% purity) and raffinose (98% purity) were purchased from Sigma (St. Louis, MO) and used without further purification. Oligosaccharide solutions (5.0×10^{-4} M in 50:50% vol., water: acetonitrile and 2 mM sodium chloride) were infused through the capillary tip using similar flow rates.

Results and Discussion

OMS Distributions for Ubiquitin. Figure 2 shows OMS distributions for the $[M+9H]^{9+}$, $[M+10H]^{10+}$, and $[M+11H]^{11+}$ charge states of electro sprayed ubiquitin ions that are obtained by scanning the drift field application frequency from 0 to 55000 Hz. For individual charge states, the most intense peak is observed as the lowest frequency feature corresponding to ion transmission in the f_i range. The peaks in the fundamental region are centered at $f_i = 1470$, 1455, and 1470 Hz for the $[M+9H]^{9+}$, $[M+10H]^{10+}$, and $[M+11H]^{11+}$ charge states, respectively. Overtone frequency peaks are observed over a wide frequency range. The $37 \cdot f_i$ overtone peak is the highest frequency OMS distribution peak observed in the range studied here.

In general, as the frequency is increased, a more complicated pattern of overtone peaks of decreasing intensities is observed.

For example, the $[M+9H]^{9+}$ charge state shows only a single feature in the relatively narrow frequency range corresponding to f_i . However, two features are observed in the $5 \cdot f_i$ region. We also observe that the intensities of higher-frequency peaks decrease. Additionally, the OMS resolving power ($R_{OMS} = f/\Delta f$) improves in higher overtone regions.^{1,2} For example, a very high R_{OMS} value of 220 was obtained at the $33 \cdot f_i$ overtone peak (47820 Hz) for the $[M+11H]^{11+}$ charge state ions of ubiquitin. The origin of increasing R_{OMS} with increasing frequency is discussed elsewhere.² The loss in signal intensity at successive higher overtone frequency regions has been ascribed to ion diffusion, and depletion due to losses associated with operation at higher overtone numbers.² In OMS experiments, these factors coupled with the use of wire mesh grids limit the overall ion signal. Of note is that the specification for 90% transmittance grids is an optical transmittance value and under the relatively high-pressure conditions of the drift tube greater ion loss may occur. That said, one advantage of the OMS method is that, as opposed to IMS which utilizes discrete packets of ions, OMS imposes a mobility filter on ions originating from a continuous beam. The experiments performed here demonstrated sufficient ion signals to obtain OMS distributions up to the $37 \cdot f_i$ region. Current studies are focused on the use of a circular drift tube geometry^{54,55} that can be used to

perform OMS separations employing dynamic fields without requiring grids on drift tube lenses.

The OMS distributions gradually change in terms of the resolved species in the high frequency region. Consider the $[M+11H]^{11+}$ ions. By the $17 \cdot f_i$ region, two features are resolved at field application frequencies of 23470 and 24280 Hz. In the $21 \cdot f_i$ region, the intensity ratio of lower to higher frequency peaks decreases. This is slightly reversed from the $29 \cdot f_i$ to $33 \cdot f_i$ regions. The $[M+9H]^{9+}$ and $[M+10H]^{10+}$ ions show the resolution of multiple species upon reaching the $5 \cdot f_i$ region. These multiple features are preserved at higher overtone frequency regions (i.e., the $9 \cdot f_i$ to the $21 \cdot f_i$ and the $9 \cdot f_i$ to the $29 \cdot f_i$ regions for the $[M+9H]^{9+}$ and $[M+10H]^{10+}$ ions, respectively). However, single features are observed for these ions at the highest OMS frequencies. Below, we present a model that describes the origin of the observed OMS distribution changes.

OMS Distributions for Substance P, Melezitose, and Raffinose. Although we do not show the distribution, the OMS spectrum recorded over the f_i region for substance P ions shows two distinct features corresponding to the $[M+3H]^{3+}$ and $[M+2H]^{2+}$ ions as confirmed by mass spectrometry analysis. Single features have been observed for the $[M+H]^+$ ions of the oligosaccharides melezitose and raffinose. Here, we note that, because data

TABLE 1: Comparison of OMS and IMS Cross Sections

ions	OMS ccs ^a (Å ²)										IMS ccs (Å ²)
	$m^b = 1$	$m = 5$	$m = 9$	$m = 13$	$m = 17$	$m = 21$	$m = 25$	$m = 29$	$m = 33$	$m = 37$	
ubiquitin [M+5H] ⁵⁺	966.9	1019.6	1013.0								1045 ^c
ubiquitin [M+6H] ⁶⁺	1092.3	1012.0	1015.9								1004 ^c
ubiquitin [M+7H] ⁷⁺	1109.0	1058.8	1059.9								1050 ^c
		1053.2	1056.4								1050 ^c
		1099.1	1092.2								1113 ^c
		1287.2	1328.2								1258 ^c
		1541.9	1554.9								
ubiquitin [M+8H] ⁸⁺	1371.6	1228.6	1384.2								1063 ^c
		1374.1	1713.1								1217 ^c
		1714.1									1367 ^c
											1670 ^c
											1695 ^c
ubiquitin [M+9H] ⁹⁺	1531.8	1746.0	1471.3	1472.2	1531.8	1750.9	1748.5	1742.5	1744.1	1738.1	1500 ^c
		1534.7	1508.8	1518.2	1742.4						1733 ^c
			1741.2	1743.1							
ubiquitin [M+10H] ¹⁰⁺	1787.9	1693.0	1682.6	1635.8	1804.2	1806.9	1808.1	1804.8	1854.5	1857.2	1590 ^c
		1791.7	1792.8	1686.9	1854.7	1857.6	1854.7	1853.7			1660 ^c
				1791.3							1790 ^c
				1852.1							1850 ^c
ubiquitin [M+11H] ¹¹⁺	1885.9	1875.7	1880.2	1882.1	1787.1	1883.4	1879.4	1881.2	1883.619		1750 ^c
				1963.2	1879.8	1950.0	1952.1	1953.7	1953.5		1879 ^c
					1944.7						1953 ^c
ubiquitin [M+12H] ¹²⁺	2009.8	2003.0	2003.9	2001.5	2000.5	1999.3	2003.0	2002.3			1767 ^c
											1845 ^c
											1998 ^c
											2072 ^c
											2115 ^c
ubiquitin [M+13H] ¹³⁺	2120.7	2124.8	2123.8	2118.2	2102.0						
substance P [M+2H] ²⁺	311.7										313.8 ^d
											285 ^e
											273 ^f
substance P [M+3H] ³⁺	321.5										319.7 ^d
melezitose [M+H] ⁺	129.8										131 ^g
raffinose [M+H] ⁺	142.9										138 ^g

^a Cross sections correspond to peak maxima in the distributions. ^b Values of m depend on the magnitude of ϕ (see text for details). ^c From ref 59. ^d Values that have been calculated from data reported previously (ref 62). ^e From ref 63. ^f From ref 60. ^g Values as measured on a prototype 3 m drift tube (not published).

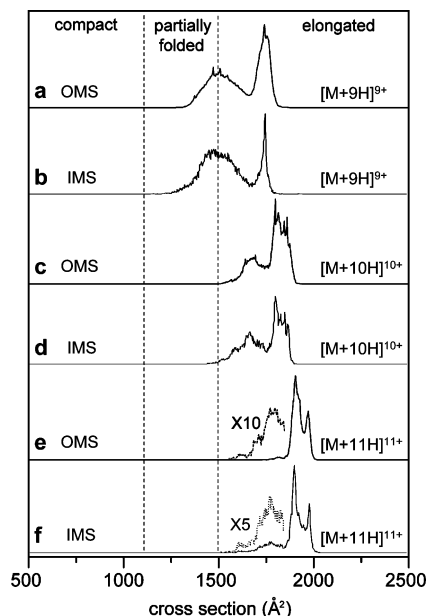


Figure 3. Cross section distributions for the $[M+9H]^{9+}$ to $[M+11H]^{11+}$ charge states of ubiquitin ions obtained from OMS (a, c, and e) and IMS (b, d, and f) measurements. For OMS distributions, the $9\cdot f_i$, $13\cdot f_i$, and $17\cdot f_i$ overtone spectra have been chosen for the $[M+9H]^{9+}$, $[M+10H]^{10+}$, and $[M+11H]^{11+}$ ions, respectively. Regions divided by dashed lines correspond to compact, partially folded, and elongated conformations, as defined previously.⁵⁶ IMS distributions are obtained by taking slices from a two-dimensional $t_D(m/z)$ data set. The OMS distributions are plotted by determining the cross sections from overtone frequencies, eq 1.

sets for these species were only recorded in the f_i region, relatively broad peaks have been obtained. Although peak centers have been used to obtain collision cross section measurements, it is not possible to draw conclusions about the numbers of stable conformations for these ions. The data are reported here to provide additional comparisons to IMS measurements.

Collision Cross Sections from OMS Measurements. Table 1 lists the collision cross sections that have been obtained from OMS data sets of the protein ubiquitin, the peptide substance P, and the oligosaccharides melezitose and raffinose. It is instructive to compare cross sections obtained from OMS measurements with those obtained from IMS experiments, which are also included in Table 1. For ubiquitin ions, the comparison is achieved by selecting overtone regions exhibiting collision cross section distributions that most closely resemble those obtained from IMS. Figure 3 shows a comparison of cross section distributions for the $[M+9H]^{9+}$ to $[M+11H]^{11+}$ ions from OMS and IMS measurements. Consider the distribution of the $9\cdot f_i$ overtone region for the $[M+9H]^{9+}$ ubiquitin ions (Figure 3). The IMS distribution for this charge state shows a population of structures existing over a broad range in size (from ~ 1150 to ~ 1660 Å²). A sharp peak is also observed at $\Omega = 1733$ Å². Similarly, the $9\cdot f_i$ overtone spectrum displays a broad distribution that includes a range of partially folded conformations and a single narrow peak at $\Omega = 1741$ Å². The peak intensity ratios for the broad and narrow features are similar ($\sim 1:2$) for the OMS and IMS distributions. OMS and IMS collision cross section distributions of the $[M+10H]^{10+}$ and $[M+11H]^{11+}$ ubiquitin ions are also very similar (Figure 3). This similarity in collision cross section distribution exists over a limited field application frequency range; for this instrument, the OMS measurement at low field application frequencies (f_i and $5\cdot f_i$) does not have the required resolving power to distinguish peaks to the same degree the high-resolution IMS

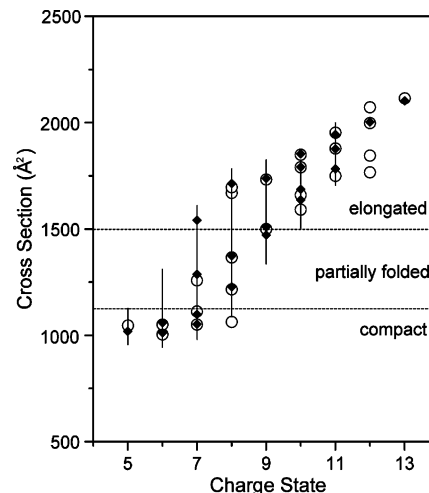


Figure 4. Cross sections for the $[M+5H]^{5+}$ to $[M+13H]^{13+}$ charge state ions of ubiquitin. The open circles correspond to data recorded using IMS.⁵⁹ The solid diamonds indicate data obtained by OMS. The vertical lines show a range of cross sections that are associated with unresolved conformations. Dashed lines indicate divisions for compact, partially folded, and elongated conformational states. Different overtone spectra for individual charge states have been analyzed to calculate the cross sections (the $5\cdot f_i$ overtone spectra for the $[M+5H]^{5+}$ to $[M+8H]^{8+}$ ions, the $9\cdot f_i$ overtone spectrum for the $[M+9H]^{9+}$ ions, the $13\cdot f_i$ overtone spectrum for the $[M+10H]^{10+}$ ions, and the $17\cdot f_i$ overtone spectra for the $[M+11H]^{11+}$ to $[M+13H]^{13+}$ ions).

measurement does. At higher field application frequency settings, the OMS collision cross section distribution is once again dissimilar to the IMS distribution, as ions undergoing structural changes are eliminated (see explanation below).

The general agreement in collision cross sections obtained from OMS and IMS⁵⁶ measurements for what appears to be similar conformations of ubiquitin ions observed in both data sets can be observed by examining Figure 4. For given charge states, corresponding structures observed with OMS have nearly identical collision cross section distributions as those observed in IMS distributions. There are instances where specific conformational types are observed for one technique but are not present in the other (see, for example, the $[M+7H]^{7+}$, $[M+8H]^{8+}$, and $[M+12H]^{12+}$ ions in Figure 4). The origin of some differences in OMS distributions is discussed below. However, in general, the agreement between OMS and IMS collision cross sections for peaks that are observed in both techniques is good. In general, comparison of any OMS cross section with an IMS value for the same conformer shows agreement to within $\pm 1\%$ relative uncertainty. Thus, the OMS approach is a reliable means of obtaining cross sections. The good agreement in collision cross sections also suggests that the dynamic nature of OMS drift fields as well as the highly repulsive fields in the d_c regions do not significantly alter the mobilities of the ions.

Evidence for Structural Changes. Figure 5 shows cross section distributions for the $[M+9H]^{9+}$ charge state ions obtained at each of the frequency regions (f_i and $m = 5$ to 37) studied here. At the f_i setting, a broad, unresolved distribution of conformations is observed extending from $\Omega \approx 1100$ to 2000 Å². When the field application frequency range is increased to the $5\cdot f_i$ region, two features of equal intensity are present in the spectrum. A broad feature of unresolved, partially folded structures is observed over the cross section range of $\Omega \approx 1300$ – 1660 Å². The second, narrower feature corresponds with ions having a collision cross section of $\Omega = 1741$ Å². As the field application frequency range is increased to the $9\cdot f_i$ region,

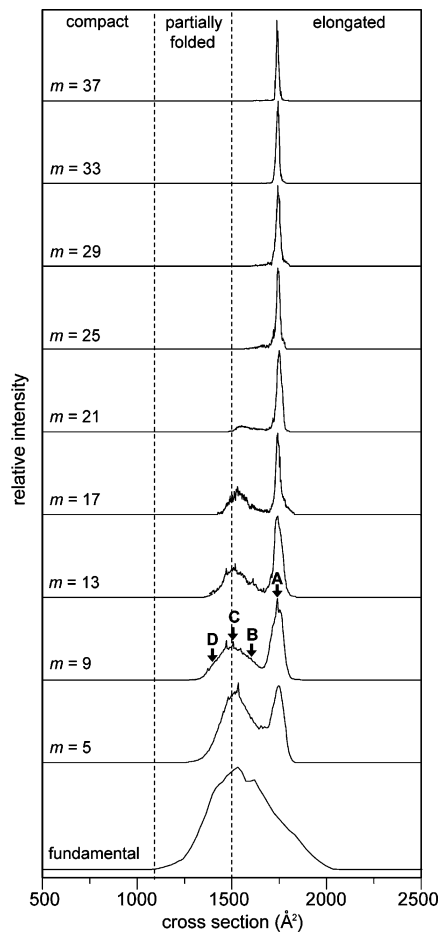


Figure 5. Cross section distributions for the $[M + 9H]^{9+}$ charge state of electro sprayed ubiquitin ions obtained from OMS measurements. The OMS spectrum has been recorded from the f_i to the $37 \cdot f_i$ overtone. m indicates the harmonic frequency number allowing the ion transmission. Dashed lines indicate divisions for compact, partially folded, and elongated conformational states. Four conformations (labeled A, B, C, and D, $\Omega = 1417, 1508, 1612,$ and 1741 \AA^2 , respectively) have been chosen to simulate structural transitions (see Figures 6 and 7 and the text for details).

the intensity level of the broad feature decreases relative to the more elongated conformation. In the $13 \cdot f_i$ and $17 \cdot f_i$ regions, a greater valley is observed between the two data set features, indicating a more rapid loss of ions with conformations of sizes intermediate to the partially folded and elongated conformations. Additionally, ions with the smallest conformations are also lost. The feature representing the elongated conformation also becomes narrower. As the field application frequency is increased to the $21 \cdot f_i$ region, a large decrease in the proportion of the partially folded states is observed. In the $25 \cdot f_i$ and $29 \cdot f_i$ regions, only the largest partially folded states remain. Upon reaching the $33 \cdot f_i$ regions, only the most elongated conformation persists. The data set feature corresponding to this conformation continues to narrow from the $25 \cdot f_i$ region to the $37 \cdot f_i$ region.

In addition to the distributions described in each of the overtone frequency regions described above, additional data set features are observed between the f_i and $5 \cdot f_i$ frequency regions. These distributions are similar to those observed in the $5 \cdot f_i$ regions for all three charge states. These features have been observed previously in OMS measurements and are more prevalent in operational modes employing larger values of ϕ .² In general, such peaks are more highly resolved and appear to

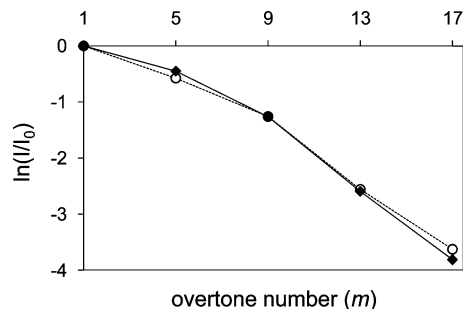


Figure 6. Plot of calculated (\blacklozenge) and experimental (\circ) relative intensity ratios as a function of m for the elongated conformation (labeled A in Figure 5) of the $[M+9H]^{9+}$ charge state of ubiquitin ions. Relative intensities obtained from ion trajectory simulations were calculated accounting for a contribution from ion diffusion but excluding structural transitions.

belong to a separate overtone series. Because the origin of these peaks is currently under investigation, they will not be discussed further here.

Ion Trajectory Simulations. In order to understand the evolution of the OMS distributions with increasing overtone frequency, it is useful to consider that the physical size of the transmissible portion of the ion beam decreases with increasing frequency.² Species that undergo structural transitions may be eliminated at some overtones but not others. That is, the stable region of the ion beam is a factor of 37 times shorter for the $37 \cdot f_i$ overtone peak than for the f_i . Because of this, the rates that structures change will influence the spectrum differently for different overtone regions. These changes in OMS distributions in different frequency regions can be modeled theoretically to bracket the kinetics associated with these changes. Here, we present three models describing possible structural transitions for ubiquitin.

In this analysis, the simulation monitors the time-dependent displacement of individual ions. The total displacement per time step is calculated by summing the contributions from the electric field as well as random variations associated with diffusion. The electric field at each ion location point is obtained from field array files similar to that produced by Simion.⁵⁷ Because experiments have been carried out using a four-phase ($\phi = 4$) system, four separate field array files are used. Each contains repulsive fields in a unique set of d_e regions signaling ion neutralization. The accumulated drift time and user-defined field application frequency dictates which field array file is used for each time step displacement calculation.

Initially, the algorithm selects one field array file and reads in the four array points immediately surrounding the two-dimensional position of the ion. Using the distance of the ion to each point, a weighted-average field is then calculated for both the x - and y -dimensions representing the field at the ion location. The drift velocity of the ion ($v = KE$) as well as the defined time step (typically $\leq 2 \mu\text{s}$) is then used to calculate the displacement of the ion resulting from its mobility.

Displacement of ions due to diffusion is simulated by considering the root-mean-square displacement of the ion as given by³⁸

$$\sqrt{r^2} = (4D\Delta t)^{1/2} \quad (5)$$

Δt represents the user-defined time increment. Ion diffusion coefficients can be obtained using the mobilities of the ions ($D = k_bTK/e$). For these studies, K is obtained from the experi-

mentally determined values in the OMS instrument for the $[M+9H]^{9+}$ ubiquitin ions. To randomize the contribution to ion displacement in two dimensions due to diffusion, $(\overline{r^2})^{1/2}$ is converted into a polar coordinate vector by randomizing a single angle (Θ). It is straightforward to use $(\overline{r^2})^{1/2} \cdot \sin \Theta$ and $(\overline{r^2})^{1/2} \cdot \cos \Theta$ to represent the y - and x -axis vector components, respectively. Thus, ion diffusion can range from $-(\overline{r^2})^{1/2}$ to $(\overline{r^2})^{1/2}$ in each dimension for each time step. This displacement due to diffusion is then added to that from the mobility calculation to produce a net ion displacement for each time increment. Ion trajectory simulations using this treatment for diffusion show that with the use of a sufficient number of separate calculations (separate ions) Gaussian shaped peaks of the appropriate width are produced for model ion packets. Additionally, the modeling of diffusion in this manner leads to the accurate representation of the dependence of ion intensity on field application frequency for OMS experiments.²

For the calculations, ions originate in positions that are referenced with respect to the $d_i(1)$ region immediately preceding the first ion elimination region [$d_e(1)$]. These regions are equal in size to all other d_i and d_e regions. The same total number of d regions (22) is used for the simulation and the experiment. The $d_i(1)$ region is 354 grid units long, and the trajectories for 10 ions beginning at each grid unit are determined, resulting in a total of 3540 separate calculations.

Kinetics Models. The simplest model simulated for structural transitions is that a conformer C changes into a conformer C', where C' has an off-resonant mobility with respect to the field application frequency. Structural transformations are considered to occur as a first order reaction where the residual starting conformation is determined according to⁵⁸

$$I = I_0 e^{-kt} \quad (6)$$

Here, I and I_0 represent the intensity of C for given experiments and the initial intensity of C, respectively. These values are obtained from peak heights in the experimental data sets (see Figure 5) and from the numbers of transmitted ions of a population for respective frequency settings in the simulations. Here, we note that a more accurate treatment of the data would be to utilize peak areas. However, because individual conformations are not resolved in the partially folded region of the OMS distribution (Figure 5), this is currently not possible for this system. The first-order rate constant, k , corresponds to conversion of C into conformer C'. The second model takes into account structural transformations approaching equilibrium where C changes into C' which can subsequently change back into conformer C. Here, the amount of the initial conformation is determined according to⁵⁸

$$I = \frac{k_2 + k_1 e^{-(k_2+k_1)t}}{k_2 + k_1} I_0 \quad (7)$$

where k_1 and k_2 represent the rate constants for the forward and reverse reactions, respectively (see below for more details). For all simulations reported here, ion mobilities have been varied by $\pm 4\%$. That is, the ratio of the size of C to C' is 1.04. We note that smaller and larger variations were tested and did not fit the experimental data as well.

Simulation Results. For this analysis, it is important to begin by understanding the ion losses that are due to diffusion alone for a stable state that undergoes no structural changes during the measurement. The elongated conformer (labeled A in Figure 5, $K = 0.0795 \text{ m}^2 \cdot \text{V}^{-1} \cdot \text{s}^{-1}$) persists to the highest frequency regions for the $[M+9H]^{9+}$ ubiquitin ions, albeit at reduced intensity levels. Ion trajectory simulations for loss of the elongated form of conformer A include losses from ion diffusion (see above) but exclude structural transitions (mobility variation). Figure 6 shows that the decrease in the calculated intensity with increasing frequency is nearly identical to the decrease observed experimentally. This is consistent with a peak centered at 1741 \AA^2 that corresponds to a relatively stable elongated conformer (or set of similar stable conformers). All of the ion losses with increasing overtone number can be ascribed to losses expected from diffusion alone.

As shown in Figure 5, the broad feature corresponding to ions with more compact conformations is lost more rapidly with increasing overtone number than the elongated ions. Ion trajectory simulations for a select, partially folded state (labeled C in Figure 5, $K = 0.0920 \text{ m}^2 \cdot \text{V}^{-1} \cdot \text{s}^{-1}$) for the $[M+9H]^{9+}$ charge state of ubiquitin ions have been performed. Figure 7 shows a comparison of the calculated and experimental intensity ratios (I/I_0) for conformer C as a function of the harmonic number using the two different kinetics models.

For the irreversible kinetics model (Figure 7a), the rate constants tested extend over a 30-fold range. At higher rate constants, a greater number of ions exhibiting conformer C convert to conformer C' during the simulated drift time. Overall, more ions—compared with the experimental results—are neutralized in the d_e regions due to the greater time with an altered mobility. Thus, we conclude we need to tune either the rates or structures, or both. Simulations using very small rate constants show that an insufficient number of ions is eliminated. For this model, the simulation with a rate constant of 150 s^{-1} provides the best fit to the experimental data.

A reversible conformational transition has also been modeled utilizing different rate constants. Figure 7b shows the ion trajectory modeling results for the reversible system in which the conversion of conformer C' to C is equal to or slower than the process of converting from C to C'. For this analysis, k_1 was maintained at 200 s^{-1} while k_2 was varied from 50 to 200 s^{-1} (increments of 50). The modeling data utilizing $k_1 = 200 \text{ s}^{-1}$ and $k_2 = 150 \text{ s}^{-1}$ are the most similar to the experimental intensity trace. It is noteworthy that an increase of 33% in the forward reaction rate (to a value of 200 s^{-1}) requires a sizable reverse reaction rate (almost equal at 150 s^{-1}).

Another possible structural variation is that ions rapidly interconvert between two conformations. In this model, the average mobility associated with the conformational changes is set to the resonant mobility. For example, conformers C and C' are assigned mobilities that are 2% higher and lower, respectively, than the resonant mobility. If values of k_1 and k_2 are large ($>10^3$), multiple structural transformations occur for each field application setting. This ensures that the average mobility is sufficiently sampled such that most of the ions can make it through the instrument at lower and intermediate overtone frequencies. However, at higher overtone frequencies, the transmissible portion of the ion beam decreases (according to a factor of $1/m$) to a size where ions having off-resonant mobilities even for a short period of time are eliminated. Figure 7c shows that, for all values of k_1 and k_2 tested, such a fast reversible model underestimates and overestimates ion loss at low and high frequencies, respectively.

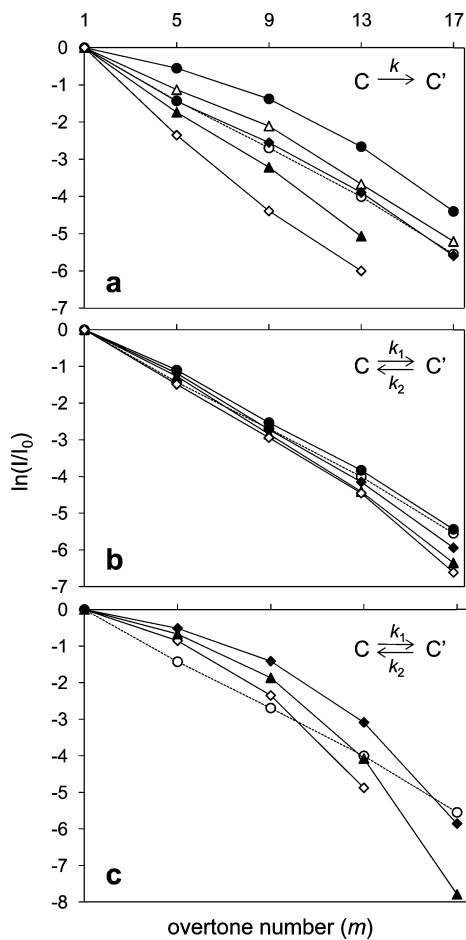


Figure 7. Plot of calculated and experimental relative intensity ratios as a function of m for a partially folded conformation (labeled C in Figure 5) of the $[M+9H]^{9+}$ charge state of ubiquitin ions. The dashed trace represents relative intensities obtained from the experimental results. Relative intensities obtained from ion trajectory simulations were calculated utilizing $\pm 4\%$ variation in mobility (see text for details). The three kinetics models used to simulate the intensities of conformer C during ion transmission are as follows: (a) an irreversible reaction (\bullet $k = 10$; \triangle $k = 100$; \blacklozenge $k = 150$; \circ exp.; \blacktriangle $k = 200$; \diamond $k = 300$); (b) a reversible reaction at relatively low rates ($k_1 = 200$ for all; \bullet $k_2 = 200$; \circ exp.; \blacklozenge $k_2 = 150$; \blacktriangle $k_2 = 100$; \diamond $k_2 = 50$); (c) a reversible reaction at relatively high rate constant ($k_1 = k_2$; \blacklozenge $k = 6932$; \circ exp.; \blacktriangle $k = 2310$; \diamond $k = 1155$).

Both the irreversible and reversible models provide reasonable fits to the experimental data. These best fits require similar rate constants (e.g., $k = 150$ and $k_1 = 200$ s^{-1} for the respective models). The half-lives (τ , where $I/I_0 = 0.5$) obtained from the best fits are $\tau \approx 4.62$ and 5.94 ms for the irreversible and reversible models, respectively. This result suggests that these ions change structures on a few millisecond time scale. This is consistent with our previous data showing structural transitions of ubiquitin ions with no activation (i.e., conformational changes were observed when a relatively unstable ion was selected).⁵⁹ Because partially folded conformations are those that undergo structural transformations, it is possible that Coulomb repulsion causes these species to gradually elongate over this time period. Previous studies have monitored the elongation of proteins and ions over tens of ms.^{3–5} This would also explain the relative stability of the elongated conformation, as the balance between Coulomb repulsion and attractive intramolecular interactions results in a more stable structure. Finally, this argument may somewhat favor the irreversible process, as such species may initially elongate minimally to relieve strong Coulomb repulsion

prior to the more extensive elongation observed previously.^{3–5} That said, the data are insufficient to rule out either process.

As a final note, the OMS distributions for the $[M+9H]^{9+}$ ubiquitin ions (Figure 5) demonstrate that structural transformations of specific partially folded conformations occur over varying time scales. It is worthwhile to consider the rates of change for other species. Simulations for conformers B and D (labeled in Figure 5, $K = 0.0883$ and 0.0998 $m^2 \cdot V^{-1} \cdot s^{-1}$, respectively) have been performed using the irreversible model system. On the basis of the modeling results, conformers B and D undergo structural transitions at a higher rate than conformer C with rate constants of 190 and 280 s^{-1} , respectively.

Conclusions

OMS measurements have been performed for a number of gas-phase ions produced by direct electrospray of ubiquitin, substance P, raffinose, and melezitose solutions. Overall, collision cross sections obtained from OMS measurements are in good agreement with those obtained by IMS. Additionally, the production of similar collision cross section distributions at specific overtone frequency regions indicates the robust nature of the OMS technique for determining ion mobilities. Modeling structural transitions by fitting experimental peak intensity ratio data obtained from OMS distributions for $[M+9H]^{9+}$ ubiquitin ions indicates that a portion of the ion population undergoes a structural transition on a few ms time scale. Because IMS measurements occur on this time scale, they do not expose these structural transitions, as drift time distributions provide the average mobilities for these ions. Such determinations are also problematic for multidimensional IMS techniques, as multiple mobility selections using variable time delays would require a substantial amount of time to monitor a single dataset feature. By allowing the tuning of the transmissible portion of the ion beam to very short lengths, OMS offers the unique advantage of elucidating such conformational changes for multiple gas-phase ions over a relatively short time period.

Acknowledgment. The authors acknowledge support in part for the development of new instrumentation by grants from the National Institutes of Health (AG-024547-01, P41-RR018942, and IRC1GM090797-01). Partial funding has also been provided by the DoD NSWC Crane “Next Generation Threat Detection” (N00164-08-C-JQ11).

References and Notes

- (1) Kurulugama, R. T.; Nachtigall, F. M.; Lee, S.; Valentine, S. J.; Clemmer, D. E. Overtone Mobility Spectrometry: Part 1. Experimental Observations. *J. Am. Soc. Mass Spectrom.* **2009**, *20*, 729–737.
- (2) Valentine, S. J.; Stokes, S. T.; Kurulugama, R. T.; Nachtigall, F. M.; Clemmer, D. E. Overtone Mobility Spectrometry: Part 2. Theoretical considerations of Resolving Power. *J. Am. Soc. Mass Spectrom.* **2009**, *20*, 738–750.
- (3) Badman, E. R.; Hoaglund-Hyzer, C. S.; Clemmer, D. E. Monitoring Structural Changes of Proteins in an Ion Trap over ~ 10 –200 ms: Unfolding Transitions in Cytochrome c Ions. *Anal. Chem.* **2001**, *73*, 6000–6007.
- (4) Myung, S.; Badman, E.; Lee, Y. J.; Clemmer, D. E. Structural Transitions of Electrosprayed Ubiquitin Ions Stored in an Ion Trap over ~ 10 ms to 30s. *J. Phys. Chem. A* **2002**, *106*, 9976–9982.
- (5) Badman, E.; Myung, S.; Clemmer, D. E. Evidence for Unfolding and Refolding of Gas Phase Cytochrome c Ions in a Paul Trap. *J. Am. Soc. Mass Spectrom.* **2005**, *16*, 1493–1497.
- (6) Fenn, J. B.; Mann, M.; Meng, C. K.; Wong, S. F.; Whitehouse, C. M. Electrospray Ionization for Mass-Spectrometry of Large Biomolecules. *Science* **1989**, *246* (4926), 64–71.
- (7) Johnson, R. S.; Martin, S. A.; Biemann, K. Collision-induced fragmentation of $(M + H)^+$ ions of peptides. Side chain specific sequence ions. *Int. J. Mass Spectrom. Ion Processes* **1988**, *86*, 137–154.
- (8) Chowdhury, S. K.; Chait, B. T. Analysis of Mixtures of Closely-Related Forms of Bovine Trypsin by Electrospray Ionization-Mass Spec-

trometry - Use of Charge State Distributions to Resolve Ions of the Different Forms. *Biochem. Biophys. Res. Commun.* **1990**, *173* (3), 927–931.

(9) Loo, J. A.; Edmonds, C. G.; Smith, R. D. Primary Sequence Information from Intact Proteins by Electrospray Ionization Tandem Mass Spectrometry. *Science* **1990**, *248*, 201–204.

(10) Winger, B. E.; Lightwahl, K. J.; Rockwood, A. L.; Smith, R. D. Probing Qualitative Conformation Differences of Multiply Protonated Gas-Phase Proteins via H/D Isotopic Exchange with D₂O. *J. Am. Chem. Soc.* **1992**, *114* (14), 5897–5898.

(11) Cheng, X. H.; Fenselau, C. Target-Capture and Ion–Molecule Reactions in High-Energy Collisions Between Protonated Polypeptide Ions and Hydrogen-Containing Target Gases. *J. Am. Chem. Soc.* **1993**, *115*, 10327–10333.

(12) Covey, T. R.; Douglas, D. J. Collision Cross Sections for Protein Ions. *J. Am. Soc. Mass Spectrom.* **1993**, *4*, 616–623.

(13) Suckau, D.; Shi, Y.; Beu, S. C.; Senko, M. W.; Quinn, J. P.; Wampler, F. M., III; McLafferty, F. W. Coexisting stable conformations of gaseous protein ions. *Proc. Natl. Acad. Sci. U.S.A.* **1993**, *90*, 790–793.

(14) Reimann, C. T.; Quist, A. P.; Kopniczky, J.; Sundqvist, B. U. R.; Erlandsson, R.; Tengvall, P. Impacts of Polyatomic Ions on Surfaces - Conformation and Degree of Fragmentation Determined by Lateral Dimension s of Impact Features. *Nucl. Instrum. Methods Phys. Res., Sect. B* **1994**, *88*, 29–34.

(15) Cox, K. A.; Julian, R. K., Jr.; Cooks, R. G.; Kaiser, R. E., Jr. Conformer Selection of Protein Ions by Ion Mobility in a Triple Quadrupole Mass Spectrometer. *J. Am. Soc. Mass Spectrom.* **1994**, *5*, 127–136.

(16) Campbell, S.; Rodgers, M. T.; Marzluff, E. M.; Beauchamp, J. L. Deuterium exchange reactions as a probe of biomolecule structure. Fundamental studies of gas phase H/D exchange reactions of protonated glycine oligomers with D₂O, CD₃OD, CD₃CO₂D, and ND₃. *J. Am. Chem. Soc.* **1995**, *117* (51), 12840–12854.

(17) Clemmer, D. E.; Hudgins, R. R.; Jarrold, M. F. Naked Protein Conformations: Cytochrome *c* in the Gas Phase. *J. Am. Chem. Soc.* **1995**, *117*, 10141–10142.

(18) von Helden, G.; Wyttenbach, T.; Bowers, M. T. Conformation of Macromolecules in the Gas Phase: Use of Matrix-Assisted Laser Desorption Methods in Ion Chromatography. *Science* **1995**, *267*, 1483–1485.

(19) Williams, E. R. Proton Transfer Reactivity of Large Multiply Charged Ions. *J. Mass Spectrom.* **1996**, *31*, 831–842.

(20) Dongre, A. R.; Jones, J. L.; Somogyi, A.; Wysocki, V. H. Influence of peptide composition, gas-phase basicity, and chemical modification on fragmentation efficiency: Evidence for the mobile proton model. *J. Am. Chem. Soc.* **1996**, *118*, 8365–8374.

(21) Vachet, R. W.; Asam, M. R.; Glish, G. L. Secondary interactions affecting the dissociation patterns of arginine-containing peptide ions. *J. Am. Chem. Soc.* **1996**, *118*, 6252–6256.

(22) Loo, J. A. Studying noncovalent protein complexes by electrospray ionization mass spectrometry. *Mass Spectrom. Rev.* **1997**, *16*, 1–23.

(23) Valentine, S. J.; Clemmer, D. E. H/D Exchange Levels of Shape-Resolved Cytochrome *c* Conformers in the Gas Phase. *J. Am. Chem. Soc.* **1997**, *119*, 3558–3566.

(24) Green, M. K.; Lebrilla, C. B. Ion–Molecule Reactions as Probes of Gas-Phase Structures of Peptides and Proteins. *Mass Spectrom. Rev.* **1997**, *16*, 53–71.

(25) Zubarev, R. A.; Kelleher, N. L.; McLafferty, F. W. Electron capture dissociation of multiply charged protein cations. A nonergodic process. *J. Am. Chem. Soc.* **1998**, *120*, 3265–3266.

(26) Hoaglund Hyzer, C. S.; Counterman, A. E.; Clemmer, D. E. Anhydrous Protein Ions. *Chem. Rev.* **1999**, *99*, 3037–3079.

(27) Stephenson, J. L.; Schaaff, T. G.; McLuckey, S. A. Hydroiodic acid attachment kinetics as a chemical probe of gaseous protein ion structure: Bovine pancreatic trypsin inhibitor. *J. Am. Soc. Mass Spectrom.* **1999**, *10* (6), 552–556.

(28) Syka, J. E. P.; Coon, J. J.; Schroeder, M. J.; Shabanowitz, J.; Hunt, D. F. Peptide and protein sequence analysis by electron transfer dissociation mass spectrometry. *Proc. Natl. Acad. Sci. U.S.A.* **2004**, *101*, 9528–9533.

(29) Gorshkov, M. P. U.S.S.R. Inventor's Certificate 966583, 1982.

(30) Purves, R. W.; Guevremont, R.; Day, S.; Pipich, C. W.; Matyjaszczyk, M. S. Mass spectrometric characterization of a high-field asymmetric waveform ion mobility spectrometer. *Rev. Sci. Instrum.* **1998**, *69*, 4094–4105.

(31) Guevremont, R. High-field asymmetric waveform ion mobility spectrometry: A new tool for mass spectrometry. *J. Chromatogr., A* **2004**, *1058*, 3–19.

(32) Shvartsburg, A. A.; Tang, K.; Smith, R. D. Understanding and designing field asymmetric waveform ion mobility spectrometry separations in gas mixtures. *Anal. Chem.* **2004**, *76*, 7366–7374.

(33) Rosell-Llompert, J.; Loscertales, J. G.; Bingham, D.; Fernandez de la Mora, J. Sizing nanoparticles and ions with a short differential mobility analyzer. *J. Aerosol Sci.* **1996**, *27*, 695–719.

(34) Kaufman, S. L.; Skogen, J. W.; Dorman, F. D.; Zarrin, F.; Lewis, K. C. Macromolecule analysis based on electrophoretic mobility in air: Globular proteins. *Anal. Chem.* **1996**, *68*, 1895–1904.

(35) Mouradian, S.; Skogen, J. W.; Dorman, F. D.; Zarrin, F.; Kaufman, S. L.; Smith, L. M. DNA analysis using an electrospray scanning mobility particle sizer. *Anal. Chem.* **1997**, *69*, 919–925.

(36) Loo, J. A.; Berhane, B.; Kaddis, C. S.; Wooding, K. M.; Xie, Y. M.; Kaufman, S. L.; Chernushevich, I. V. Electrospray ionization mass spectrometry and ion mobility analysis of the 20S proteasome complex. *J. Am. Soc. Mass Spectrom.* **2005**, *16* (7), 998–1008.

(37) Kaddis, C. S.; Lomeli, S. H.; Yin, S.; Berhane, B.; Apostol, M. I.; Kickhoefer, V. A.; Rome, L. H.; Loo, J. A. Sizing large proteins and protein complexes by electrospray ionization mass spectrometry and ion mobility. *J. Am. Soc. Mass Spectrom.* **2007**, *18*, 1206–1216.

(38) Revercomb, H. E.; Mason, E. A. Theory of Plasma Chromatography Gaseous Electrophoresis - Review. *Anal. Chem.* **1975**, *47*, 970–983.

(39) Mason, E. A.; McDaniel, E. W. *Transport Properties of Ions in Gases*; Wiley: New York, 1988.

(40) Shvartsburg, A. A.; Jarrold, M. F. An exact hard-spheres scattering model for the mobilities of polyatomic ions. *Chem. Phys. Lett.* **1996**, *261*, 86–91.

(41) Mesleh, M. F.; Hunter, J. M.; Shvartsburg, A. A.; Schatz, G. C.; Jarrold, M. F. Structural information from ion mobility measurements: effects of the long-range potential. *J. Phys. Chem.* **1996**, *100*, 16082–86.

(42) Wyttenbach, T.; von Helden, G.; Batka, J. J.; Carlat, D.; Bowers, M. T. Effect of the long-range potential on ion mobility measurements. *J. Am. Chem. Soc.* **1997**, *8*, 275–82.

(43) Wittmer, D.; Luckenbill, B. K.; Hill, H. H.; Chen, Y. H. Electrospray Ionization Ion Mobility Spectrometry. *Anal. Chem.* **1994**, *66*, 2348–2355.

(44) Gillig, K. J.; Ruotolo, B.; Stone, E. G.; Russell, D. H.; Fuhrer, K.; Gonin, M.; Schultz, A. J. Coupling High-Pressure MALDI with Ion Mobility/Orthogonal Time-of Flight Mass Spectrometry. *Anal. Chem.* **2000**, *72*, 3965–3971.

(45) Hoaglund, C. S.; Valentine, S. J.; Sporleder, C. R.; Reilly, J. P.; Clemmer, D. E. Three-Dimensional Ion Mobility/TOFMS Analysis of Electrosprayed Biomolecules. *Anal. Chem.* **1998**, *70*, 2236–2242.

(46) Hoaglund-Hyzer, C. S.; Li, J.; Clemmer, D. E. Mobility Labeling for Parallel CID of Ion Mixtures. *Anal. Chem.* **2000**, *72*, 2737–2740.

(47) Tang, K.; Shvartsburg, A. A.; Lee, H. N.; Prior, D. C.; Buschbach, M. A.; Li, F. M.; Tolmachev, A. V.; Anderson, G. A.; Smith, R. D. High-Sensitivity Ion Mobility Spectrometry/Mass Spectrometry Using Electrodynamic Ion Funnel Interfaces. *Anal. Chem.* **2005**, *77*, 3330–3339.

(48) Koeniger, S. L.; Merenbloom, S. I.; Valentine, S. J.; Jarrold, M. F.; Udseth, H. R.; Smith, R. D.; Clemmer, D. E. An IMS-IMS Analogue of MS-MS. *Anal. Chem.* **2006**, *78*, 4161.

(49) For a review of IMS techniques, see (and references therein): St. Louis, R. H.; Hill, H. H. Ion Mobility Spectrometry in Analytical Chemistry. *Crit. Rev. Anal. Chem.* **1990**, *21*, 321–355.

(50) For a review of IMS techniques, see (and references therein): Clemmer, D. E.; Jarrold, M. F. Ion Mobility Measurements and their Applications to Clusters and Biomolecules. *J. Mass Spectrom.* **1997**, *32*, 577–592.

(51) For a review of IMS techniques, see (and references therein): Bohrer, B. C.; Merenbloom, S. I.; Koeniger, S. L.; Hilderbrand, A. E.; Clemmer, D. E. Biomolecule Analysis by Ion Mobility Spectrometry. *Annu. Rev. Anal. Chem.* **2008**, *1* (10), 1–10.

(52) Kim, T.; Tolmachev, A. V.; Harkewicz, R.; Prior, D. C.; Anderson, G.; Udseth, H. R.; Smith, R. D.; Bailey, T. H.; Rakov, S.; Futrell, J. H. Design and implementation of a new electrodynamic ion funnel. *Anal. Chem.* **2000**, *72* (10), 2247–2255.

(53) Kim, T.; Tang, K. Q.; Udseth, H. R.; Smith, R. D. A multicapillary inlet jet disruption electrodynamic ion funnel interface for improved sensitivity using atmospheric pressure ion sources. *Anal. Chem.* **2001**, *73* (17), 4162–4170.

(54) Merenbloom, S. I.; Glaskin, R. S.; Henson, Z. B.; Clemmer, D. E. High-Resolution Ion Cyclotron Mobility Spectrometry. *Anal. Chem.* **2009**, *81* (4), 1482–1487.

(55) Glaskin, R.; Valentine, S. J.; Clemmer, D. E. A Scanning Frequency Mode for Ion Cyclotron Mobility Spectrometry. *Anal. Chem.*, accepted for publication.

(56) Valentine, S. J.; Counterman, A. E.; Clemmer, D. E. Conformer-Dependent Proton-Transfer Reactions of Ubiquitin Ions. *J. Am. Soc. Mass Spectrom.* **1997**, *8*, 954–961.

(57) Dahl, D. A. SIMION, version 7.0; Idaho National Engineering Laboratory: Idaho Falls, ID.

(58) Atkins, P.; de Paula, J. *Physical chemistry*, 7th ed.; Oxford University Press: 2002.

(59) Koeniger, S. L.; Clemmer, D. E. Resolution and structural transitions of elongated states of ubiquitin. *J. Am. Soc. Mass Spectrom.* **2007**, *18* (2), 322–331.

(60) Thalassinou, K.; Slade, S. E.; Jennings, K. R.; Scrivens, J. H.; Giles, K.; Wildgoose, J.; Hoyes, J.; Bateman, R. H.; Bowers, M. T. Ion mobility mass spectrometry of proteins in a modified commercial mass spectrometer. *Int. J. Mass Spectrom.* **2004**, *236* (1–3), 55–63.

(61) Julian, R. R.; Myung, S.; Clemmer, D. E. Do Homochiral Aggregates Have an Entropic Advantage. *J. Phys. Chem. B* **2005**, *109*, 440–444.

(62) Myung, S.; Lee, Y. J.; Moon, M. H.; Taraszka, J.; Sowell, R.; Koeniger, S.; Hilderbrand, A. E.; Valentine, S. J.; Cherbas, L.; Cherbas, P.; Kaufmann, T. C.; Miller, D. F.; Mechref, Y.; Novotny, M. V.; Ewing, M. A.; Sporleder, C. R.; Clemmer, D. E. Development of high-sensitivity ion trap ion mobility spectrometry time-of-flight techniques: A high-

throughput nano-LC-IMS-TOF separation of peptides arising from a *Drosophila* protein extract. *Anal. Chem.* **2003**, *75* (19), 5137–5145.

(63) Gill, A. C.; Jennings, K. R.; Wyttenbach, T.; Bowers, M. T. Conformations of biopolymers in the gas phase: a new mass spectrometric method. *Int. J. Mass Spectrom.* **2000**, *196*, 685–697.

JP1060123